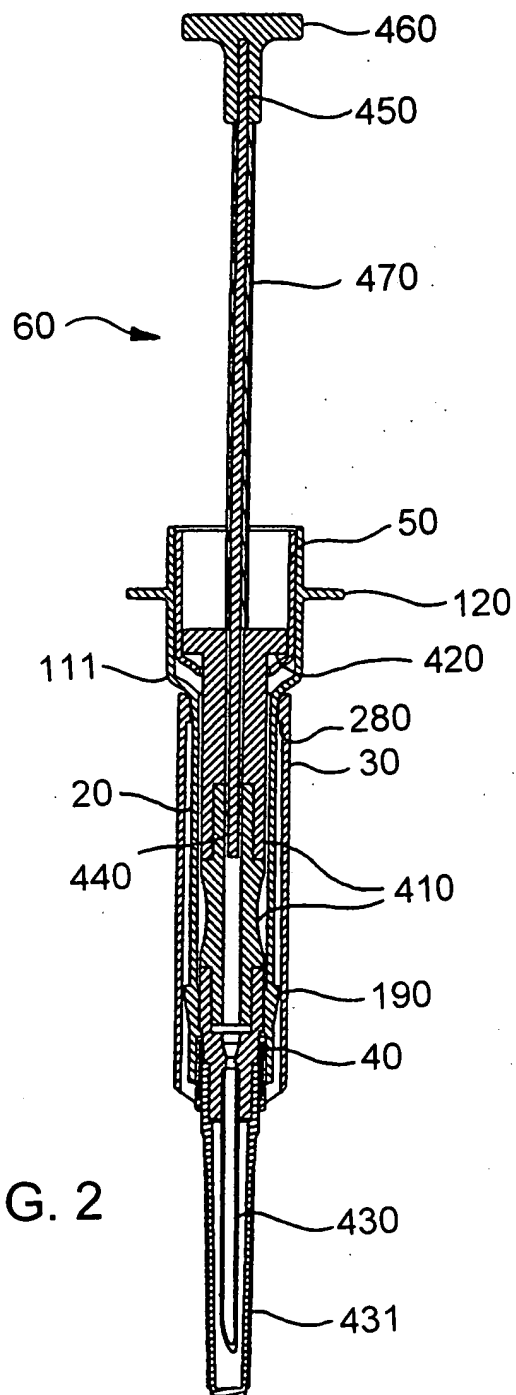
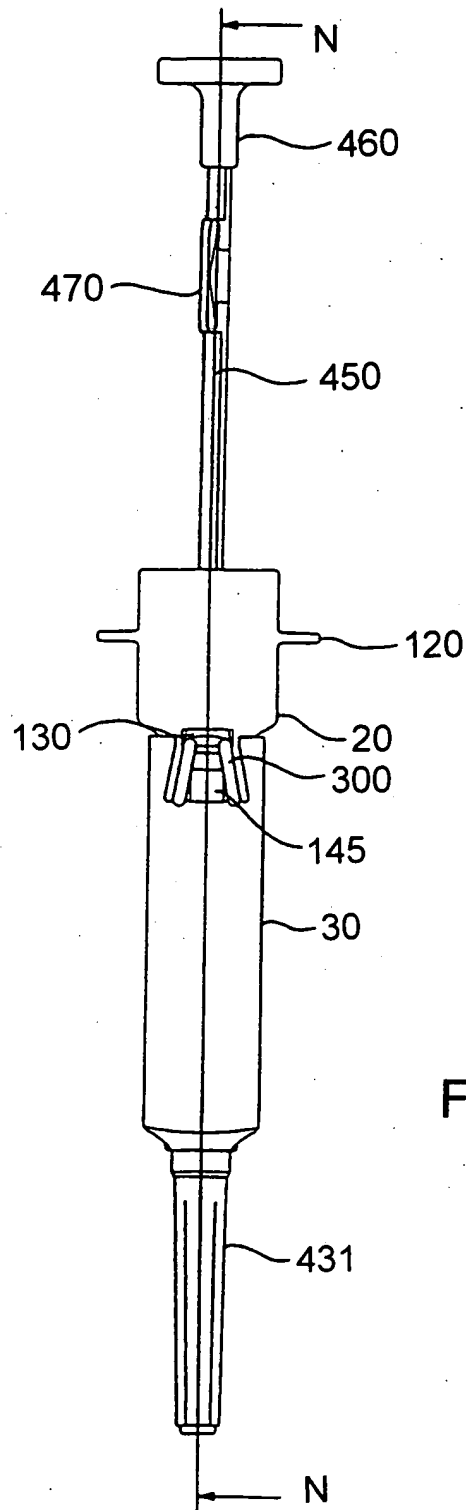
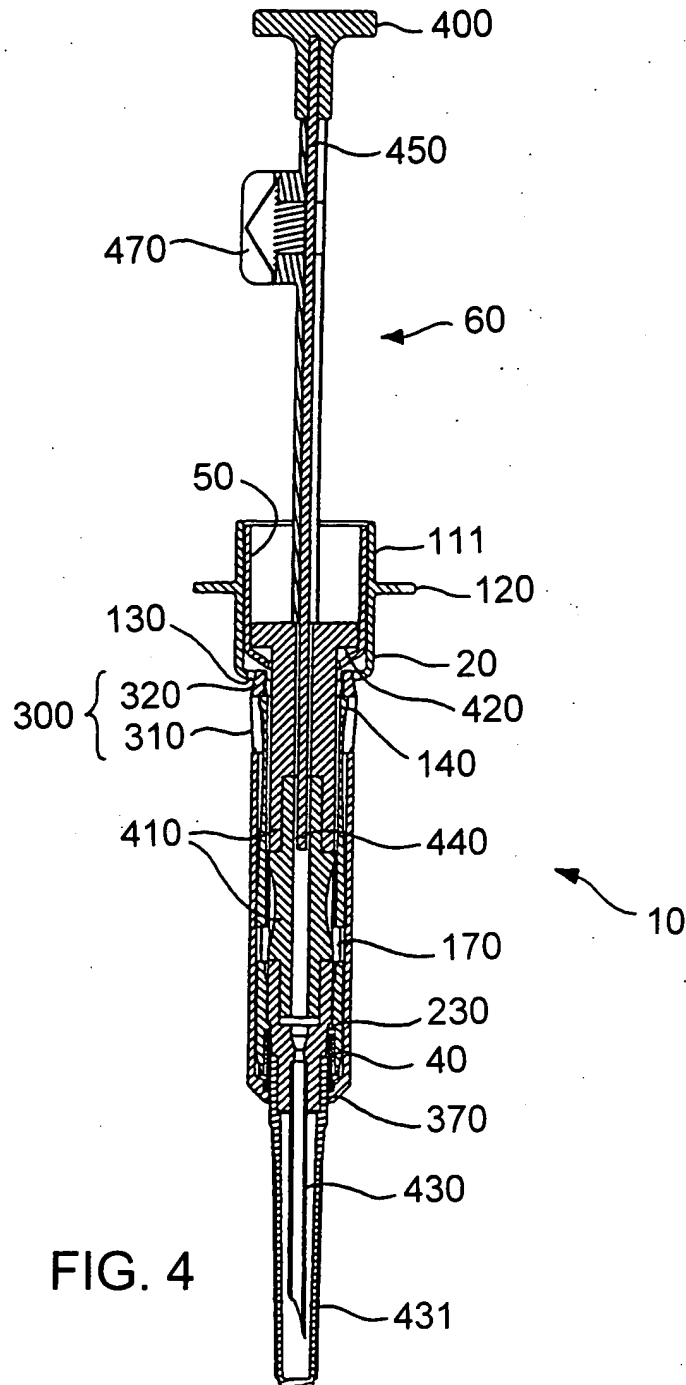



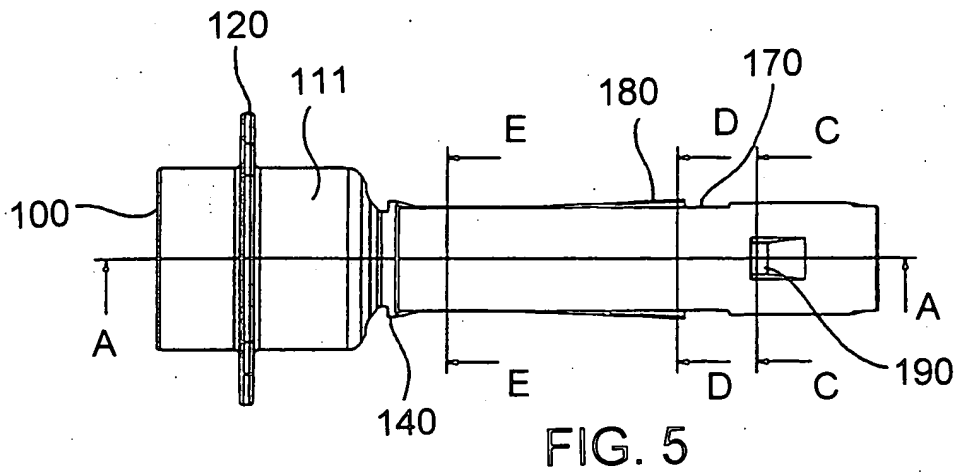


Applicant(s): Derek Shaw et al.

AUTOMATICALLY OPERABLE SAFETY SHIELD SYSTEM
FOR SYRINGES







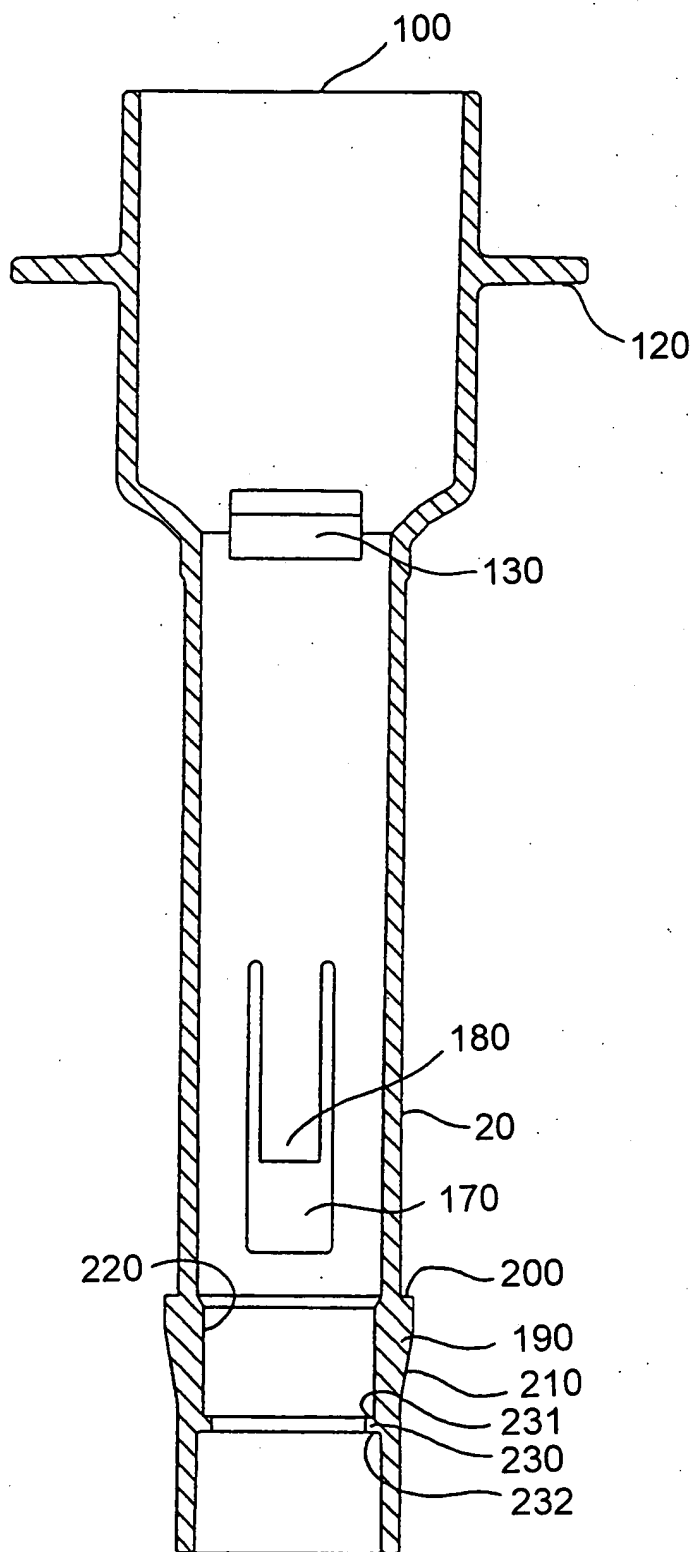
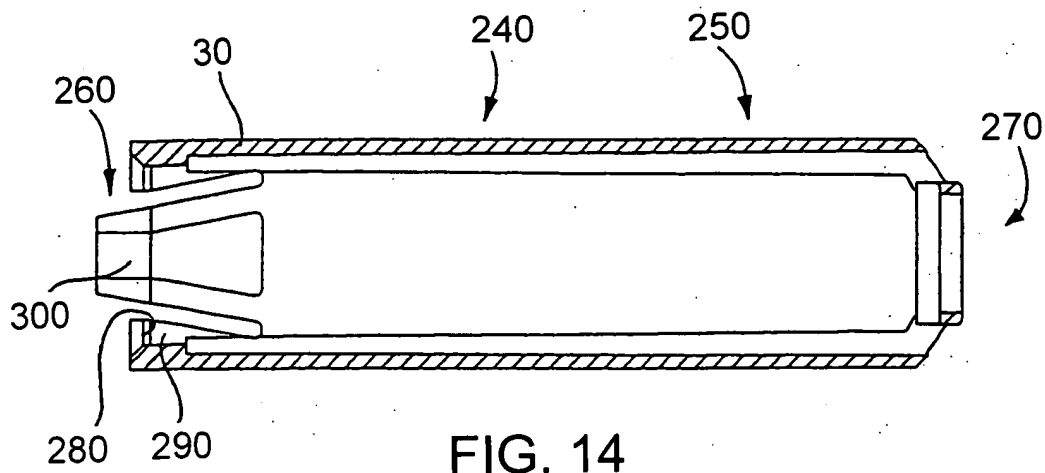
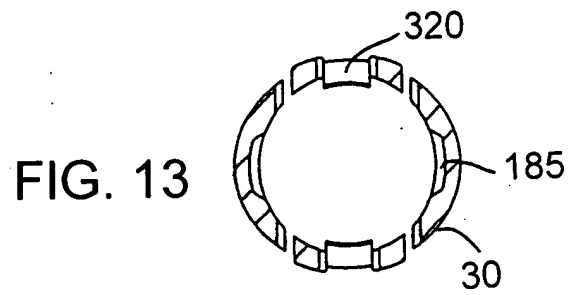


FIG. 9





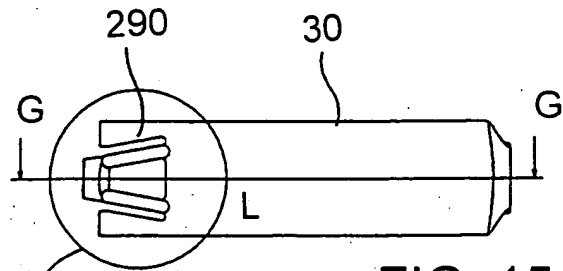


FIG. 15A

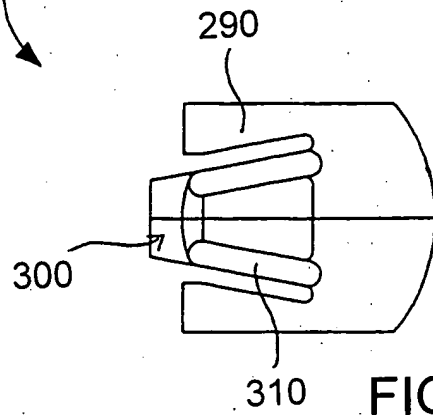
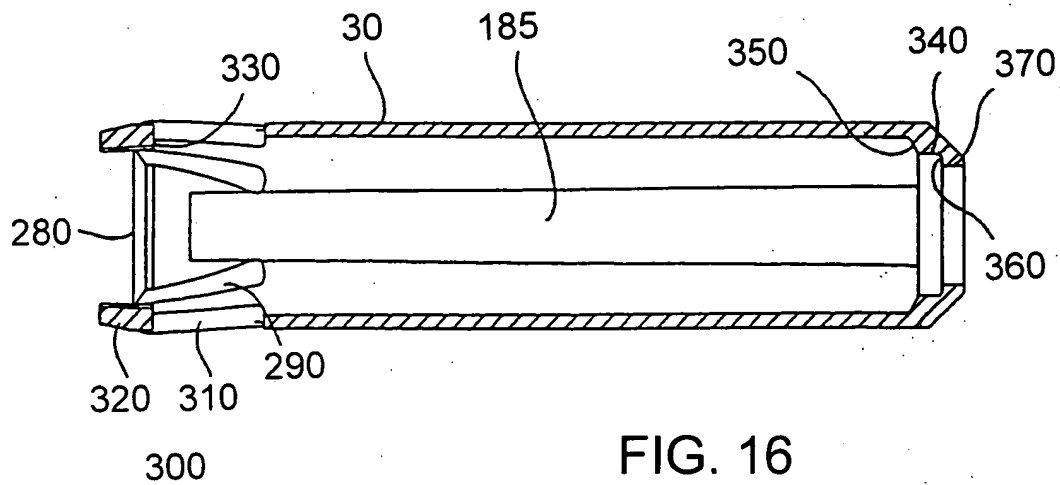
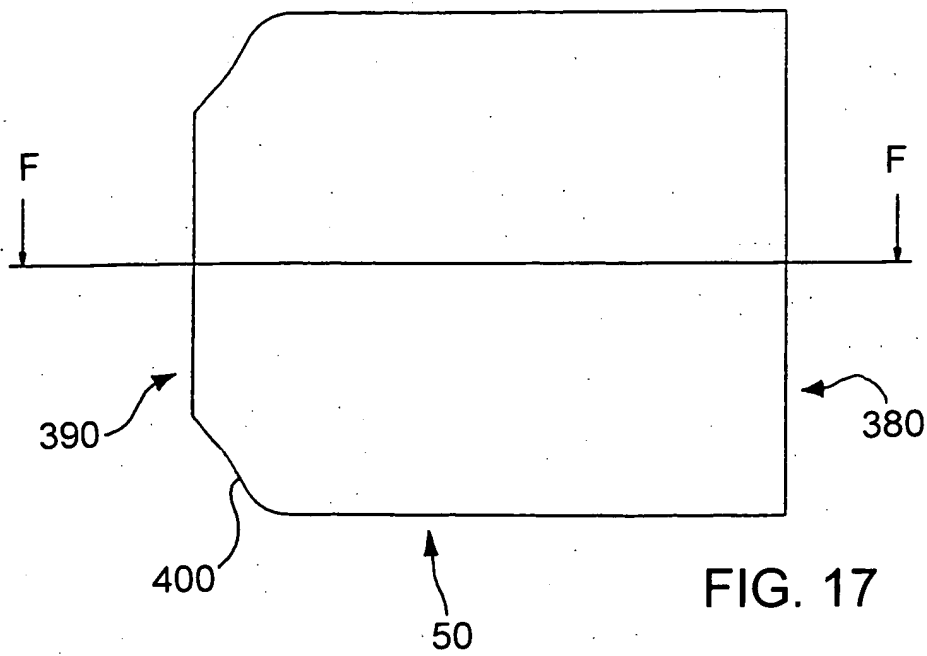
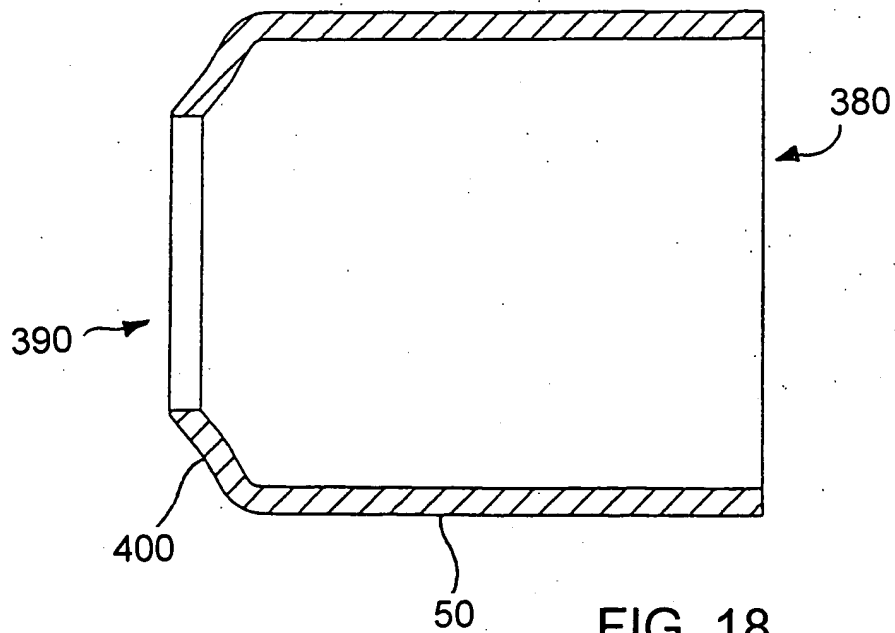


FIG. 15B







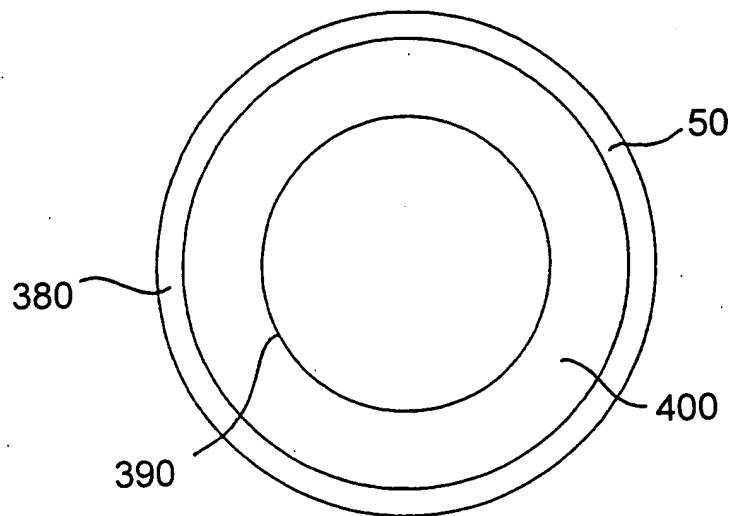
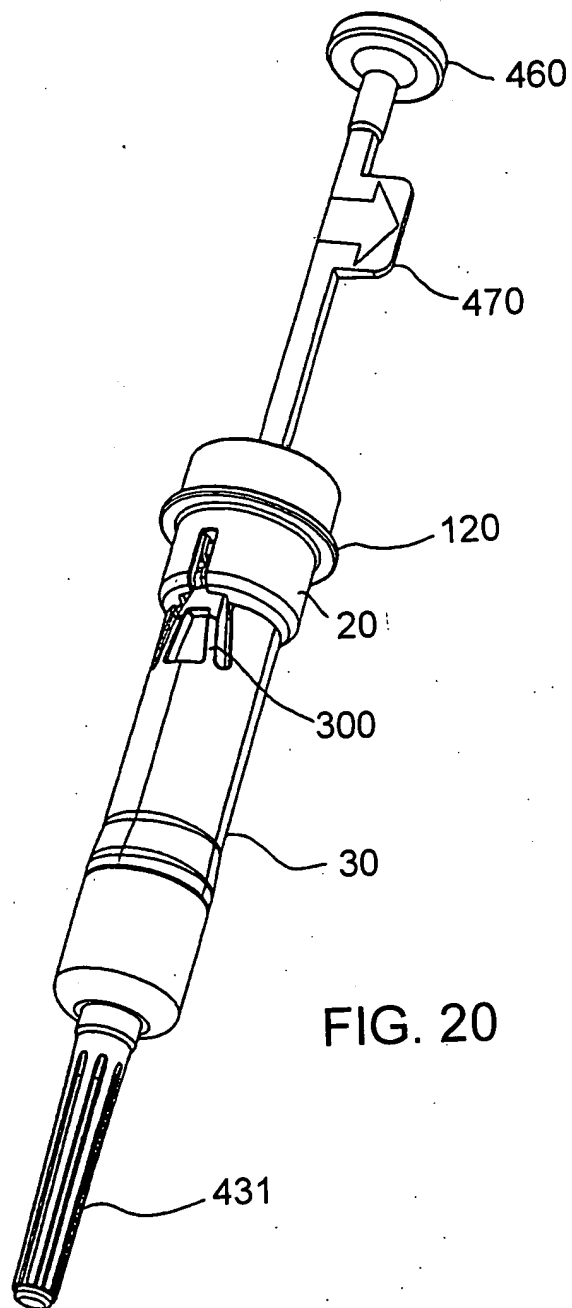
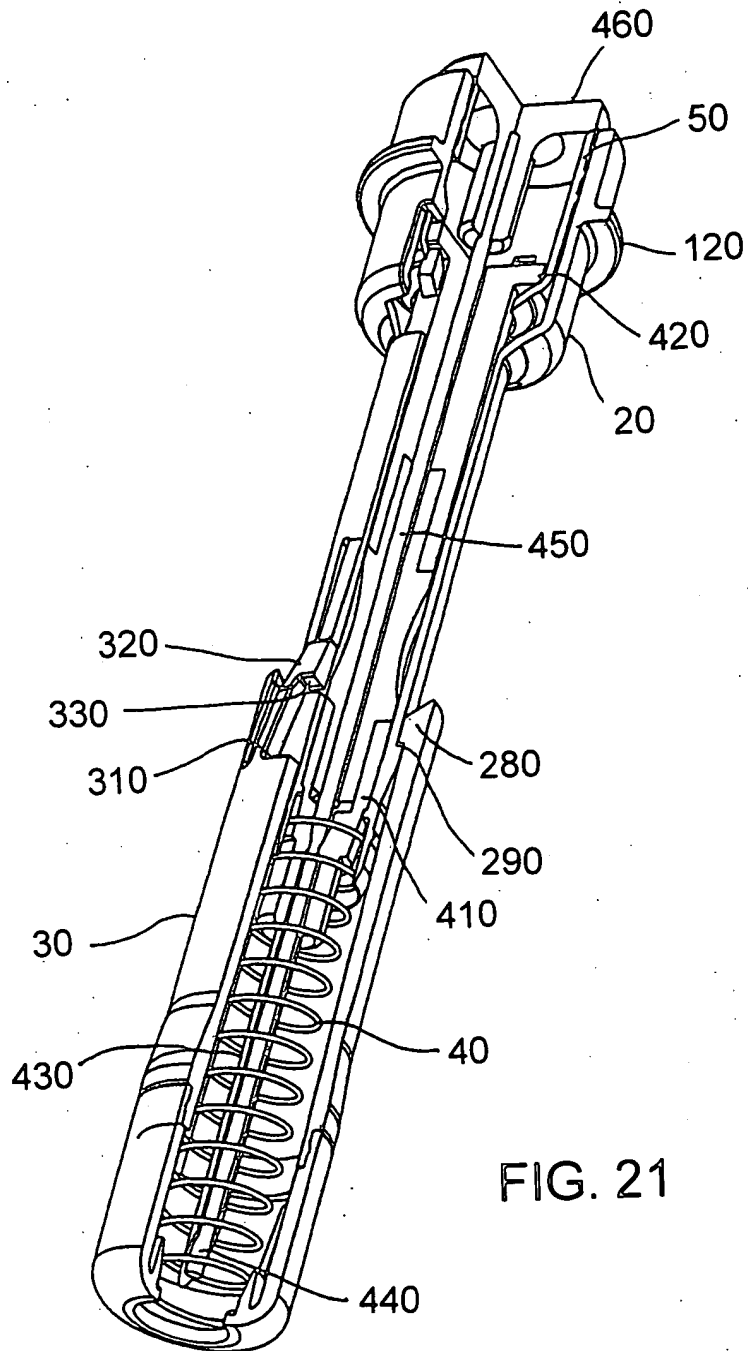
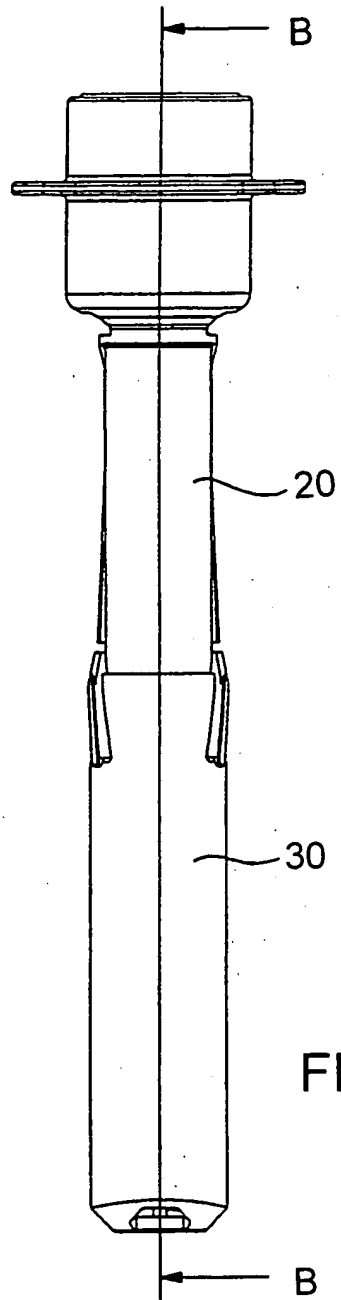


FIG. 19







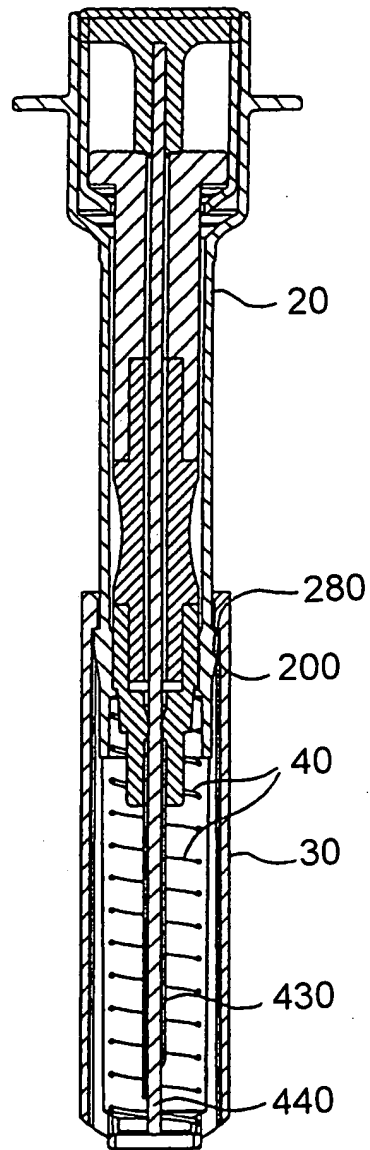
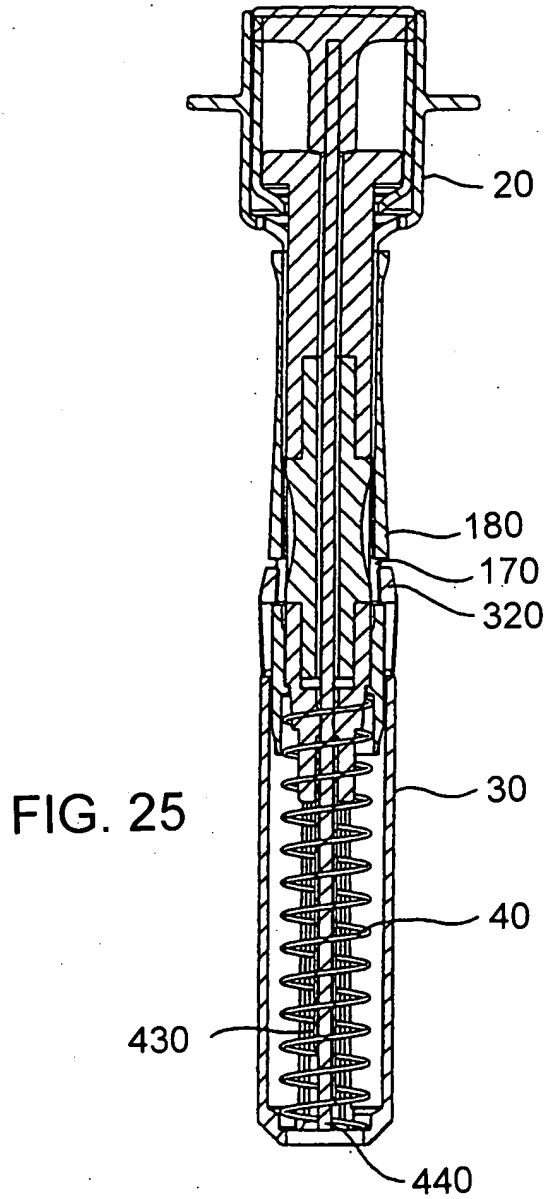


FIG. 23

FIG. 24



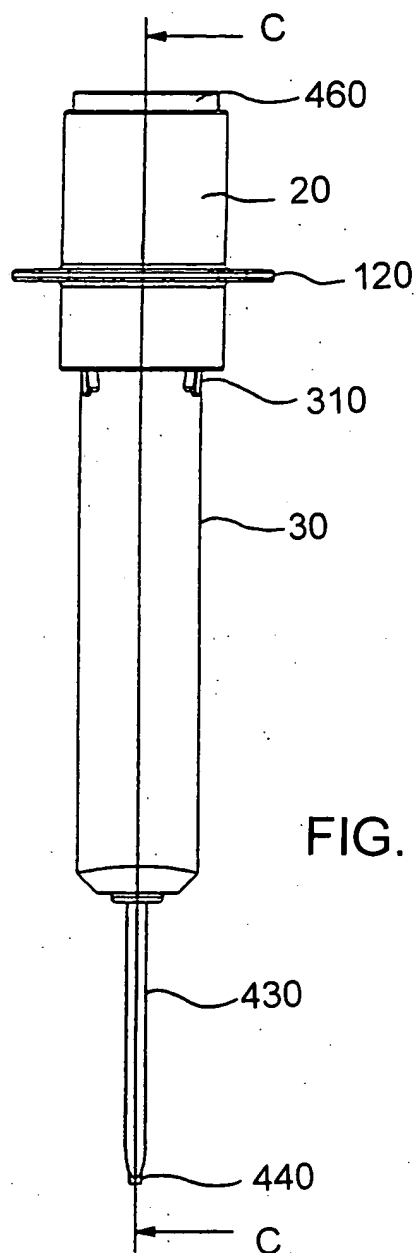


FIG. 26

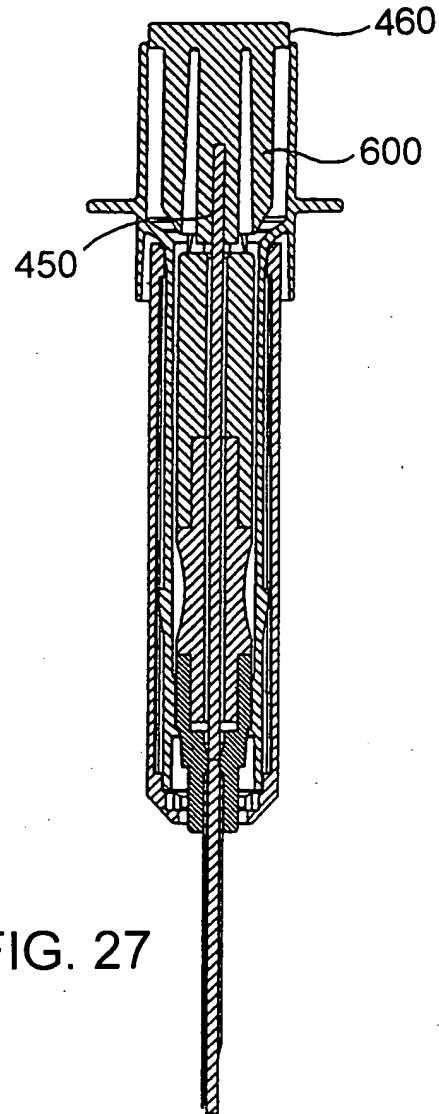
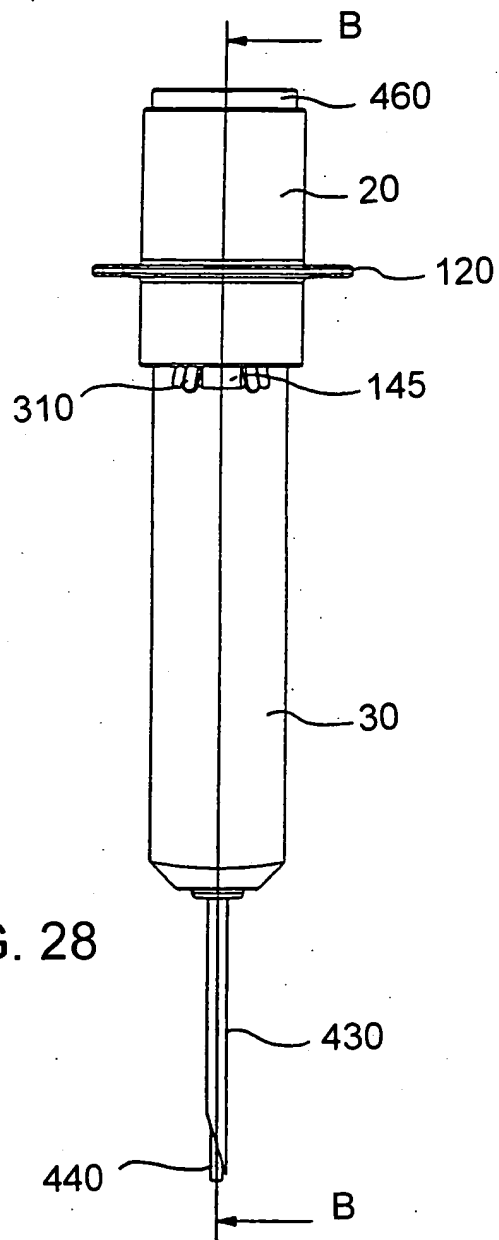


FIG. 27



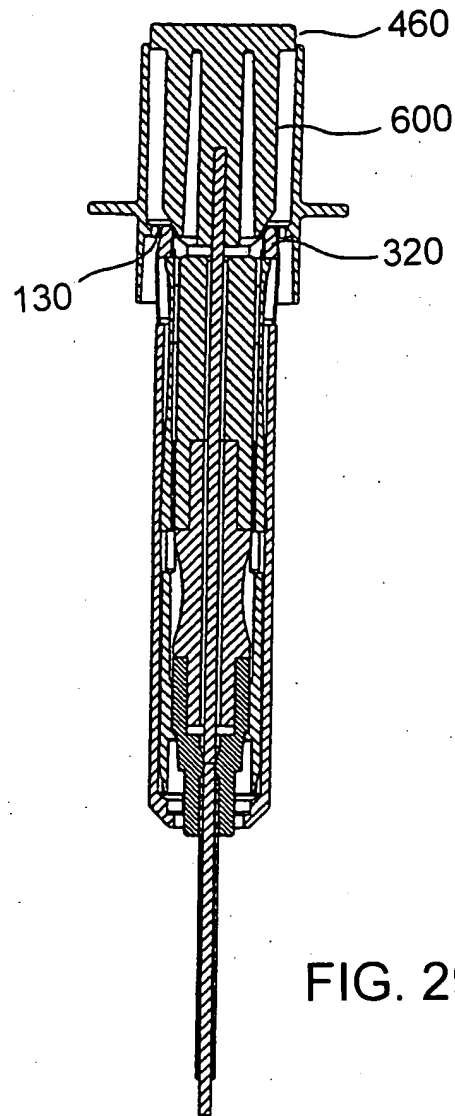


FIG. 29

